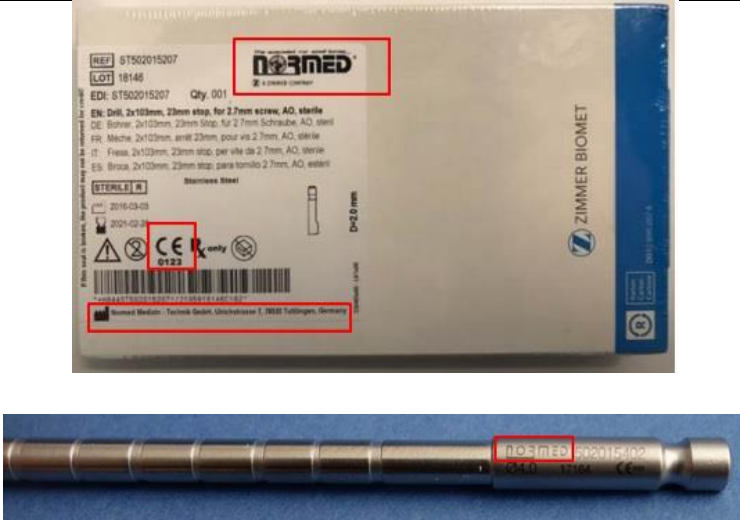


Medical Devices Safety Notice

The National Health Regulatory Authority would like to alert all governmental and private healthcare facilities, local agents and distributors that the below medical device:

| Device Details | |
|--------------------------|--|
| Device Name | Foot and Ankle Inst. (Drill / Tap and Countersink) NORMED |
| Device Model | Refer to the reference link |
| Manufacturer | Zimmer, INC |
| Country of Origin | USA |
| Reference | https://ncmdr.sfda.gov.sa/Secure/CA/CaViewRecall.aspx?caid=8&rid=14113 |
| Device picture |  |
| Reason of Recall | NHRA initiates this FSN due to tip breakages, there are certain lots manufactured by Medizin Technik GmbH using different material than defined in the applicable specifications. As a precaution the manufacturer decided to remove the complete |

For more information please contact Medical_Devices@nhra.bh

| | |
|---------------------|--|
| | family of instruments that were manufactured by Normed Medizin Technik GmbH prior to its manufacturing transfer to Zimmer Biomet in 2014. |
| Action taken | In case of having the defected medical devices, please contact your authorized representative to take the necessary action to remove the defected devices from your store. |

Your cooperation is highly appreciated in improving health services in the Kingdom of Bahrain.

For more information please contact Medical_Devices@nhra.bh